

# HPLC Analysis Report

Sample: MK-677

Batch No.: KB20141203 Mfg. Date: November 15.2014

Buffer A: 0.04% TFA in 100% water(v/v)

Buffer B: 0.04% TFA in 100% acetonitrile (v/v)


Gradient: 10-80% Buffer B in 25 min

Flow: 1ml/min Wavelength:220nm

Column: Alltima C18,4.6\*250mm,5um

Date: December 5, 2014

## Chromatogram

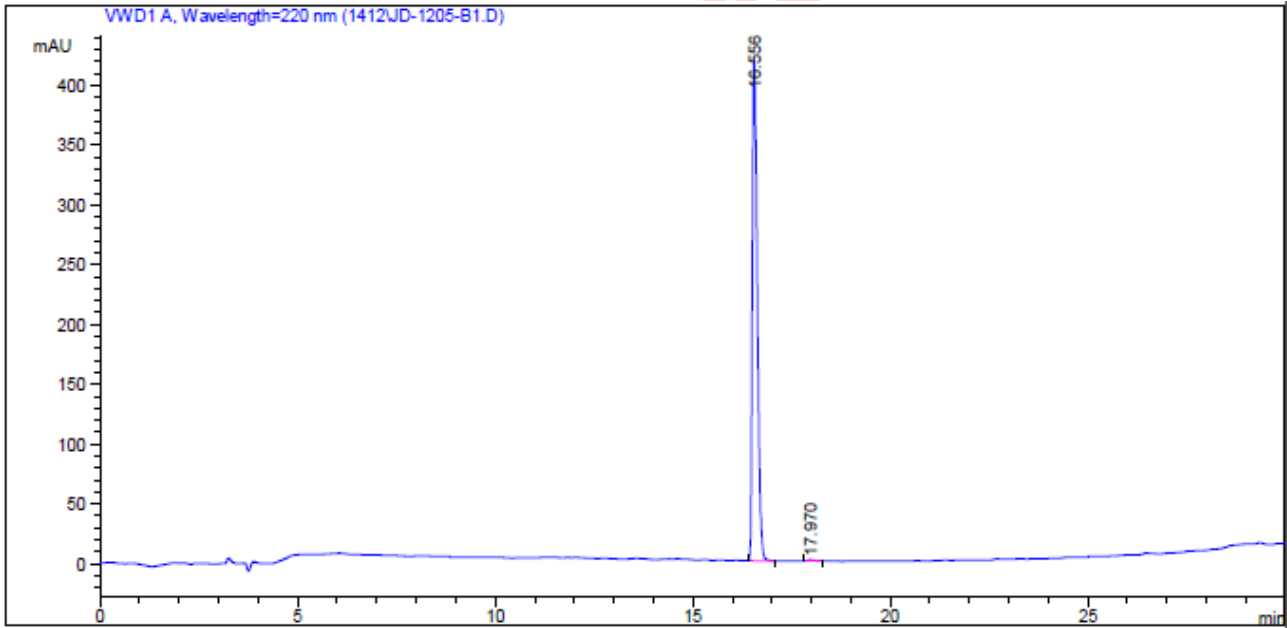

| Peak# | RetTime(Min) | Width(Min) | Area(mAU*s) | Height(mAU) | Area(%) |
|-------|--------------|------------|-------------|-------------|---------|
| 1     | 16.556       | 0.1395     | 3694.02588  | 418.12808   | 99.6295 |
| 2     | 17.970       | 0.1590     | 13.73791    | 1.24845     | 0.3705  |
| Total |              |            | 3707.76379  | 419.37653   | 100     |

Analysis Result:

Purity: 99.63%

MS Spectrum

