

HPLC Analysis Report

Sample: Raloxifene(Evista)

CAS: 84449-90-1

Batch No.: KB20141203

Mfg. Date: November 15, 2014

Buffer A: 0.04% TFA in 100% water(v/v)

Buffer B: 0.04% TFA in 100% acetonitrile (v/v)


Gradient: 10-80% Buffer B in 25 min

Flow: 1ml/min Wavelength: 220nm

Column: Alltima C18, 4.6*250mm,5um

Date: December 10, 2014

Chromatogram

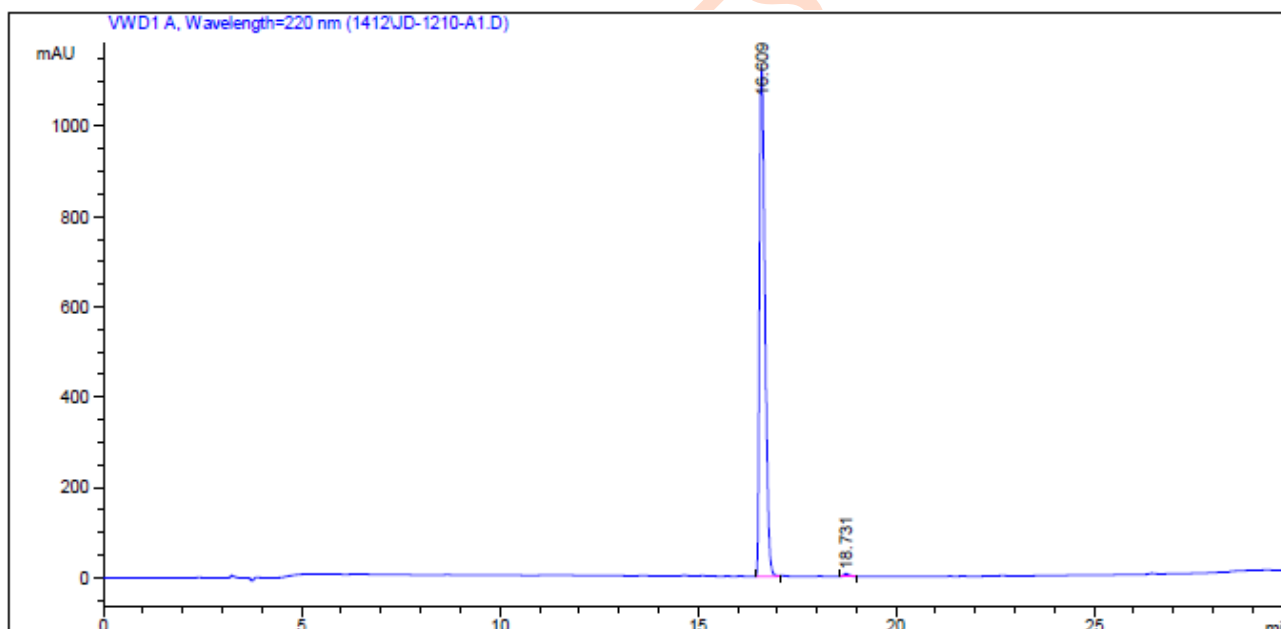

Signal Peak#	RT(min)	Width(min)	Area(mAU*s)	Height(mAU)	Area%
1	16.609	0.1497	1.07839e4	1124.78259	99.3786
2	18.731	0.1490	69.61265	6.77688	0.6414
Totals :			1.08536e4	1131.55947	100.000

Analysis Result:

Purity: 99.38%

MS Spectrum

*MSD1 SPC, time=0.309:0.709 of C:\CHEM32\1\DATA\141211\140210 2014-12-11 12-07-11\SIG1000001.D ES-API, Pos, Scan, Fr

