

# HPLC Analysis Report

Sample: SARM's S4

CAS No.: 401900-40-1

Batch No.: KB20141010

Mfg. Date: Spetmber 25,2014

Method Info: 30%-90% Buffer B 0-25 MIN

Buffer A: 0.04% TFA in 100% water(v/v)

Buffer B: 0.04% TFA in 100% acetonitrile (v/v)


Gradient: 30-90% Buffer B in 25 min

Column: Alltima C18,4.6\*250mm,5um

Flow Rate: 1mL/min

Wavelength: 220 nm

Date: October 13, 2014

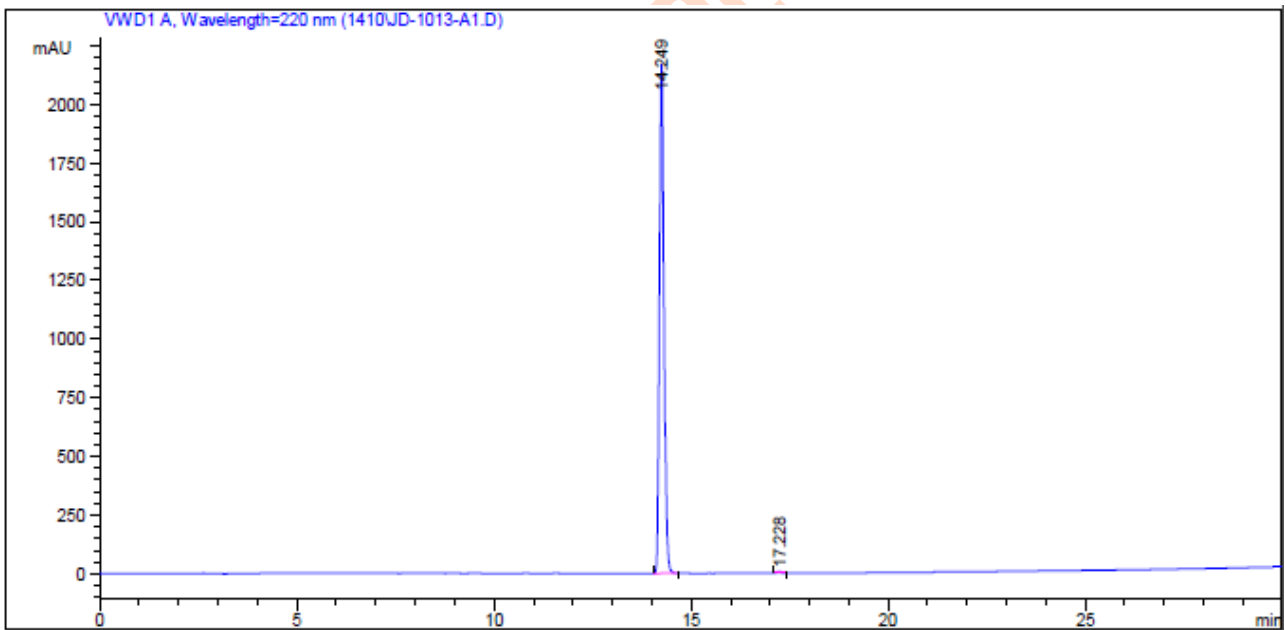

Peak#	RetTime(Min)	Width(Min)	Area(mAU*s)	Height(mAU)	Area(%)
1	14.249	0.1246	1.74888e4	2170.09399	99.8126
2	17.228	0.1193	32.83139	4.24695	0.1874
Totals			1.75216e4	2174.34094	100

Analysis Result:

Purity: 99.81%

MS Spectrum

